

No. 31286 /LGH  
To


dated Lahore the 10-4 2018

The Managing Director,  
Punjab Procurement Regulatory Authority,  
3<sup>rd</sup> Floor, Al-Falah Building, The Mall Road,  
Lahore.

Subject: **MINUTES OF TECHNICAL ADVISORY COMMITTEE MEETING**

With reference to the subject cited above.


It is therefore kindly requested to upload the minutes of Technical Advisory Committee meeting held on 29-03-2018, on official PPRA Website for the Medical Equipment & other items through regular Schemes of this hospital. (Minutes attached)

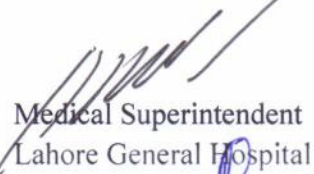  
Medical Superintendent  
Lahore General Hospital  
Lahore

No. \_\_\_\_\_ /LGH dated Lahore the \_\_\_\_\_ 2018

A copy is forwarded for information to the:-

1. Principal, PGMI/ LGH, Lahore.

  
Medical Superintendent  
Lahore General Hospital  
Lahore

# **Minutes of Technical Advisory Committee Meeting** **Held on 29-3-2018**

1. The Technical Advisory Committee meeting was held on 29-3-2018 under the chairmanship of Prof. Dr. Agha Shabbir Ali, Prof of Pediatrics, Lahore General Hospital, Lahore, regarding technical evaluation of the offers for the purchase of Medical Equipment, and sample approval of Furniture items through regular budget of this hospital.

2. Following committee members attended the meeting:-

Mr. Zia Ul Haq Tahir, Technical Officer Health  
Mr. Awais Bin Tariq, Biomedical Engineer  
Dr. Moin Nawaz, DMS Purchase  
Dr. Shabnam Gulzar, AMS (Store)  
Dr. Rakhshanda Ambreen, AMS (Equipment)  
Dr. Mehwish Murtaza, AP Plastic Surgery  
Dr. Muhammad Iqbal, Associate Prof of ENT  
Prof. Dr. Farhat Naz, Prof of Gynae  
Prof. Dr. Jodat Saleem, Prof of Anesthesia  
Prof. Dr. Khalid Waheed, Prof of Pulmonology  
Prof. Dr. M. Farooq Afzal, Prof of Surgery  
Prof. Dr. Najam Ul Hasnain, Prof of ENT  
Dr. Mahmood Salahuddin, Medical Superintendent

3. The technical sheets were prepared by the end-user & Technical Officer, Health Department, Lahore and was placed before the committee.







4. The committee decided that the clauses of tender enquiry & PPRA rules 2014, will be followed strictly.

5. The following items were discussed:-

Sr	Name of Item	Name of Firm	Remarks	Decision
1	Neonatal Ventilator	M/S Vertex Medical	The Committee decided that the said firm give the demonstration to the End-user	decision pending
		M/S Total Technologies	The Committee decided that the said firm give the demonstration to the End-user	decision pending
2	ECG Machine 12 Channel	M/S Biotech	As per Technical Specification and Bidding Documents.	Responsive
		M/S Hospicare	The said firm did not fulfill the technical evaluation criteria;- - Satisfactory Past Performance of the bidder for quoted Product not attached. - Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document not attached.	Non Responsive
		M/S Shirazi Trading	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S KASBN	As per Technical Specification and Bidding Documents.	Responsive



Sr	Name of Item	Name of Firm	Remarks	Decision
3	Steam Sterilizer + Flash Autoclave	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Clinical Life	As per Technical Specification and Bidding Documents.	Responsive
		M/S Mediland Pakistan	The Said firm did not fulfill the Technical Evaluation Criteria:- The said firm attached non Exclusive Authorization certificate	Non Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Delta Plus	The Said firm did not fulfill the Technical Evaluation Criteria:- - CE certificate of 6618 is not according to requirement.	Non Responsive
		M/S Total Technologies	As per Technical Specification and Bidding Documents.	Responsive
4	Pulse Oximeter	M/S Hospicare	The Said firm did not fulfill the Technical Evaluation Criteria:- -The said firm attached the Non Exclusive Authorization certificate instead of Exclusive/Sole Authorization agreement. - Satisfactory Past Performance of the bidder for quoted product not attached. - Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document not attached.	Non Responsive
		M/S Delta Plus	As per Technical Specification and Bidding Documents.	Responsive
		M/S Biotech	The said firm did not fulfill the Technical Evaluation Criteria:- - Satisfactory Past Performance of the bidder for quoted product not attached.	Non Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
5	Bariatric Operation Table	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Mediland Pakistan	As per Technical Specification and Bidding Documents.	Responsive
6	Operation Table for ENT, Eye and Gynae	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Eastern Medical	The said firm did not quote the Gynae Operation Table, hence not accepted.	Non Responsive
		M/S SIGMA	The said firm did not quote the Gynae Operation Table, hence not accepted.	Non Responsive

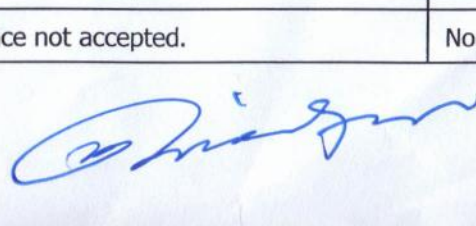

Sr	Name of Item	Name of Firm	Remarks	Decision
7	M/S Cardiac Monitor, Central Monitoring station, High End Cardiac Monitor, Central Monitor Station, High End Moduler Cardiac Monitor, Central Monitor Station.	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
8	Suction Machine Heavy Duty and Low Duty	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S KASBN	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Forcare	The Said for did not fullfill the Technical Evaluation Criteria:- - Exclusive/Sole Authorization agreement from the foreign Manufacturer not attached. - The Manufacturer should have documentary evidence to the effect that they are the original Manufacturer of the quoted product with indication of manufacturing site and its location, not attached.	Non Responsive
		M/S SIGMA	The said firm did not fullfill the Technical Evaluation Criteria:- - Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document not attached.	Non Responsive
		M/S Bestech	The said firm did not fullfill the Technical Evaluation Criteria:- -The firm submit the Non Exclusive agreement intead of Exclusive/Sole authorization agreement. -Certificate from the manufacturer that the after sales services / backup services shall be provided jointly with the local sole agent and in case of change of local agent, they will provide the after sales services themselves or through newly appointed agent for the period mentioned from the date of commissioning, not attached. -A Certificate from the manufacturer that the installation will be conducted in conformity with the system requirements by following the professional approach, not attached. -The medical equipment offered from foreign countries shall be eligible to participate and must bear FDA510k, CE(MDD) or MHLW (Ministry of Health, Labor and Welfare) standard, respectively and those products should be marketed world widely; in case the origin is not mentioned in the specifications. (The product manufactured and marketed for certain region shall be knocked down). In case of high-tech equipment, any of the above mentioned two certificates are mandatory. The country of manufacturer other than USA, Europe and Japan will be acceptable only if it is specifically mentioned in the advertised tender/Specifications, not attached.	Non Responsive



Sr	Name of Item	Name of Firm	Remarks	Decision
9	Diathermy Machine and Diathermy Machine with Vesal Ceiling.	M/S Vital Care	The Committee decided that the said firm give the demonstration to the End-user	Pending
		M/S Radiant Medical	The said firm did not fulfill the Technical Evaluation Criteria:- -The said firm submitted the Non Exclusive agreement instead of Exclusive/Sole Authorization agreement from the foreign Manufacturer. Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document not attached.	Non Responsive
		M/S Latif Brother	The Committee decided that the said firm give the demonstration to the End-user	Pending
10	OT Ceiling Light+Mobile OT Light	M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Delta Plus	As per Technical Specification and Bidding Documents.	Responsive
		M/S Eastern Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S G.Med	The said firm did not fulfill the Tender Specification:- -Electronic control panel for light field diameter and light adjustment manually adjustable is not according to specification . -Light field diameter 11-22cm instead of 15-30cm.	Non Responsive
11	BIPAP Machine Low End	M/S Med Impex	The said firm did not fulfill the Tender Specification:- -Adjustable pressure range 25cm instead of upto 30cm. -Pressure bar Graph for patient breaths and pressure not mentioned on quotation. -Temperature control Ventilation system not mentioned on quotation. -Complete with filters, carrying case and temperature controlled humidifier not mentioned on quotation.	Non Responsive
		M/S Electromed	As per Technical Specification and Bidding Documents.	Responsive
		M/S Noor International	<b>The said firm did not fulfill the Technical Evaluation Criteria:-</b> -Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document, not attached. <b>The said firm did not fulfill the Tender Specification:-</b> -Adjustable Pressure range 20cm instead of 30cm. -Pressure bar Graph for patient breaths and pressure not mentioned on quotation. -Internal/External (UPS) battery backup of two hours with complete system functionality.	Non Responsive











Sr	Name of Item	Name of Firm	Remarks	Decision
12	BIPAP Machine High End	M/S Med Impex	The said firm did not fullfill the Tender Specification:- -Adjustable pressure range 25cm instead of upto 30cm. -Pressure bar Graph for patient breaths and pressure not mentioned on quotation. -Internal/External (UPS) bettery backup of two hours with complete system functionality not mentioned on quotation. -Complete with filters, carrying case and temperature controlled humifier not mentioned on quotation.	Non Responsive
		M/S Electromed	As per Technical Specification and Bidding Documents.	Responsive
		M/S Noor International	<b>The said firm did not fullfill the Technical Evaluation Criteria:-</b> -Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document, not attached. <b>The said firm did not fullfil the Tender Specification:-</b> -Auto EPAP (AVAPS-AE) or equalant not quoted. -Adjustable Pressure rane 20cm instead of 30cm. -Pressure bar Graph for patient breaths and pressure not mentioned on quotation. -Internal/External (UPS) battery backup of two hours with complete system functionality is not mentioned.	Non Responsive
13	Anesthesia Machine Low End. Anesthesia Machine high end Anesthesia Machine high end fully Digital	M/S Shirazi Trading	The said firm did not fullfill the tender specification:- Anesthesia Machine High End -Integrated heated breathing system, not mentioned on Brochure. -Battery backuo of at least 60 minutes, not mentioned on Brochure. Anesthesia Machine High End fully Digital -Integrated heated breathing system, not mentioned on Brochure. -Battery Backup of at least 60 minutes, not mentioned on Brochure.	Non Responsive
		M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
14	Pulmonary Function Monitoring Device	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
15	Blood Warming Apparatus	M/S Medi Urge	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
16	Laposcopic Ultrasound	M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive

Handwritten signatures and initials in blue ink at the bottom of the page, including a large signature on the right and several smaller initials on the left.



Sr	Name of Item	Name of Firm	Remarks	Decision
16	Laposcopic Ultrasound	M/S Medfort	<p>The said firm did not fullfill the Technical Evaluation Criteria:-</p> <ul style="list-style-type: none"> <li>-Exclusive/Sole Authorization Agreement from the foreign Maanufacturer not attached.</li> <li>-The Manufacturer should have documentary evidence to the effect that they are the original Manufacturer of the quoted product with indication of manufacturing site and its location, not attached.</li> <li>-Certificate from the manufacturer that the after sales services / backup services shall be provided jointly with the local sole agent and in case of change of local agent, they will provide the after sales services themselves or through newly appointed agent for the period mentioned from the date of commissioning, not attached.</li> <li>-A Certificate from the manufacturer that the installation will be conducted in conformity with the system requirements by following the professional approach, not attached.</li> <li>-Satisfactory Past Performance of the bidder for quoted product, not attached.</li> <li>-The firm must have all kind of testing and calibration equipment which is required to maintain the products which they are dealing. The list of all required testing equipment will be provided along with the bid including its model number and serial numbers. The available testing equipment must be calibrated. The offers without non-availability of required testing equipment will be straightaway rejected, not attached.</li> <li>-Submission of valid legally enforceable exclusive authorization letter of manufacturer assuring full guarantee and warranty obligations as per enclosed manufacturer authorized form with the bid document, not attached.</li> <li>-Quality assurance certificate not attached.</li> <li>-The quoted model of imported product shall be available on the current official website of the manufacturer; otherwise the quoted product shall be considered obsolete/ redundant and will straight away be rejected, not mentioned.</li> <li>-The firms shall also declare the make, model, country of origin of all accessories to be provided with equipment, not mentioned.</li> <li>-An affidavit from bidder of Rs.20/- stating that their firm is not blacklisted by any of the Federal and Provincial Government or Organization of the state/Central Government in Pakistan.</li> </ul>	Non Responsive
17	Vaccum Extractor	M/S Vertex Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S KASBN	As per Technical Specification and Bidding Documents.	Responsive
		M/S Radiant Medical	As per Technical Specification and Bidding Documents.	Responsive
		M/S Forcare	<p>The said firm did not fullfill the Technical Evaluation Criteria:-</p> <ul style="list-style-type: none"> <li>-Exclusive/Sole Authorization Agreement from the foreign Maanufacturer not attached.</li> </ul>	Non Responsive
18	Hand Held Nerve Stimulator	M/S Cardiac Care	As per Technical Specification and Bidding Documents.	Responsive

Sr	Name of Item	Name of Firm	Remarks	Decision
19	Furniture Items	M/S Orient Medical	Following Sample Approved:- Office Chair, Office Table, Wheel Chair, Iron Cupboard, Dressing Trolley, Dust Bin with Lid. Following Sample Not Approved:- Computer Chair, Laptop Trolley	Responsive
		M/S Apex	The said firm not submit the samples for sample Sample Approval.	Non Responsive
		M/S Qazzafi Surgical	Following Sample Approved:- Wheel Chair, Dressing Trolley, Dust Bin with Lid, Laptop Trolley. Following Sample Not Approved:- Office Chair, Iron cupboard. Following Sample Not Provided:- <u>Office Table, Computer Chair</u>	Responsive
		M/S Medi Source	Following Sample Approved:- Office Chair, Dust Bin with Lid, Computer Chair. Following Sample Not Approved:- Office Table, Iron Cupboard. Following Sample Not Provided:- <u>Wheel Chair Heavy Duty, Dressing Trolley, Laptop Trolley.</u>	Responsive
		M/S Medi Urge	The said firm not submit the samples for Sample Approval.	Responsive
		M/S Startek	Following Sample Not Approved:- Office Chair, Office Table, Iron Cupboard, Dust Bin with Lid, Laptop Trolley. Following Sample Not Provided:- <u>Wheel Chair, Dressing Trolley, Computer Chair</u>	Non Responsive
		M/S Bestech	Following Samples Approved:- Office Chair. Following Sample Not Provided:- Office Table, Wheel Chair, Dust Bin with Lid, Iron Cupboard, Dressing Trolley, Laptop Trolley. Following Sample Not Approved:- Computer Chair,	Responsive
20	Iron Rack	M/S Bari Engineering	The sample of the firm not as per Tender specification.	Non Responsive
		M/S Techno Grip	The sample of the firm not as per Tender specification.	Non Responsive
		M/S Nine Star	The said firm not submit the sample for sample approval.	Non Responsive
		M/S Apex Enterprises	As per Technical Specification and Bidding Documents.	Responsive

P.L.  
A

*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*



Sr	Name of Item	Name of Firm	Remarks	Decision
21	Polythin Bag White	M/S M. Amir & Co	The Greviance committee reffered back the case to Technical Advisory committee to re-evaluate the sample. The Technical Advisory Committee re-evaluate the sample and found that the sample of the firm poor quality. Sample not Approved.	Non Responsive

7. The Technical Advisory Committee forwarded the case to the purchase committee to proceed further accordingly for technically approved/ decided items.

Mr. Zia Ul Haq Tahir, Technical Officer Health

Mr. Awais Bin Tariq, Biomedical Engineer

Dr. Moin Nawaz, DMS Purchase

Dr. Shabnam Gulzar, AMS (Store)

Dr. Rakhshanda Ambreen, AMS (Equipment)

Dr. Mehwish Murtaza, AP Plastic Surgery

Dr. Muhammad Iqbal, Associate Prof of ENT

Prof. Dr. Farhat Naz, Prof of Gynae

Prof. Dr. Jodat Saleem, Prof of Anesthesia

Prof. Dr. Khalid Waheed, Prof of Pulmonology

Prof. Dr. M. Farooq Afzal, Prof of Surgery

Prof. Dr. Najam Ul Hasnain, Prof of ENT

Dr. Mahmood Salahuddin, Medical Superintendent

Prof. Dr. Agha Shabbir Ali, Prof of Peads.